


Comparison of the Performance of the Colorimetric Ames MPF Assay with the Agar Plate Method

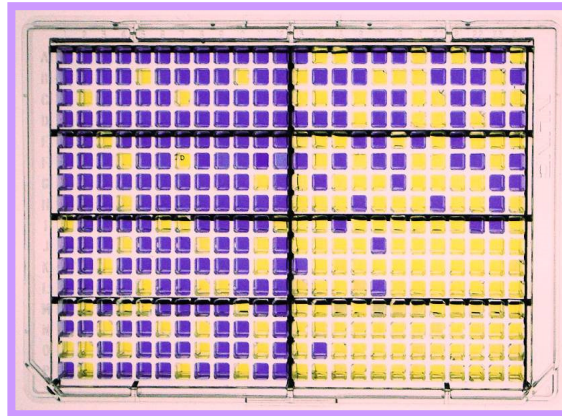


Nicole Weiland, Xenometrix AG

April 2016

Copyright Xenometrix AG

Ames MPF and Ames agar plate test

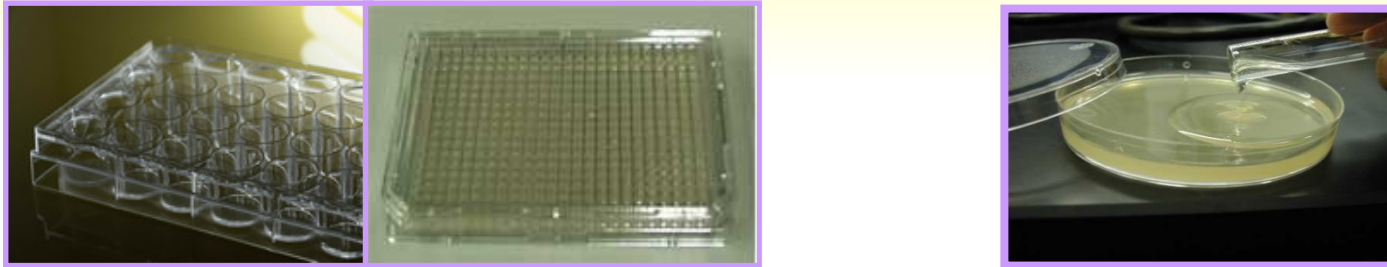

Ames MPF is based on same principle as agar plate test but

- Liquid low-volume format
- Use of microplates and multichannel pipettes
- Colorimetric read-out
- Less test sample - up to 4 fold
- Less S9 – up to 12 fold
- Higher throughput

Ames Microplate Assay Procedure

Bacterial stock
-80°C



Overnight culture



37°C, 12-15 h
250 rpm




OD₆₀₀

Assay preparation

a) Test sample dilutions, controls




b) Exposure medium
Bacterial culture +/- S9 mix

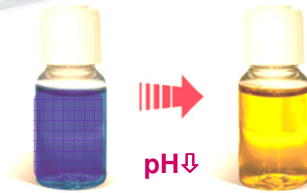

pH↓

384-well plates

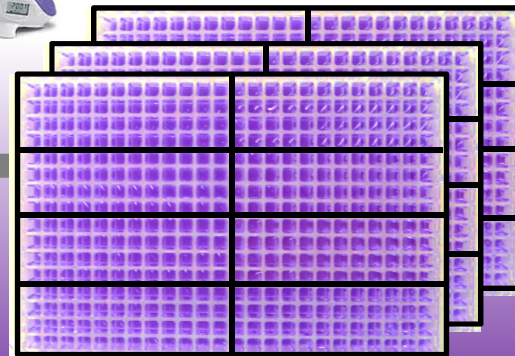


Exposure cultures

replicates 1 replicates 2 replicates 3


	1	2	3	4	5	6
A	C-	D4	C-	D4	C-	D4
B	D1	D5	D1	D5	D1	D5
C	D2	D6	D2	D6	D2	D6
D	D3	C+	D3	C+	D3	C+

37°C, 90 min, 250 rpm
(20 min E.coli +S9)

Indicator medium

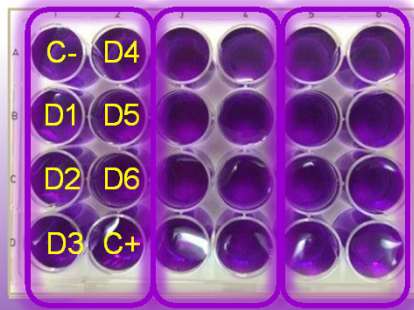


48 h, 37°C

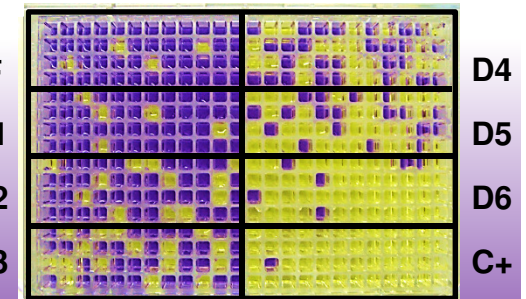

Measuring Points

Agar Plate test

- 1 plate - 1 measuring point
- Individual handling:
1 plate requires mixing of
1 compound, agar and plating

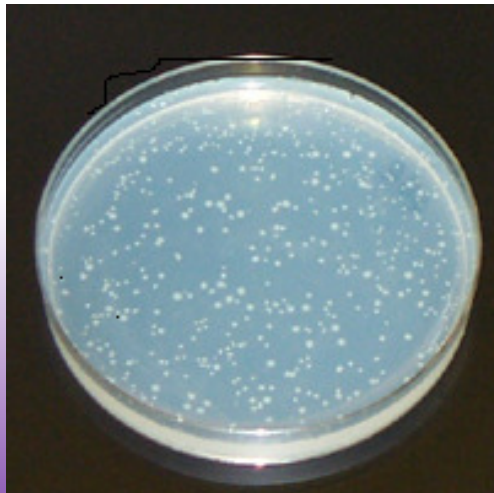

liquid culture Ames MPF

- 1 plate - 24 measuring points
- Simultaneous handling of several replicates




Evaluation of Results

Agar Plate Test vs Ames MPF


Colony counting of individual plates
Automation possible

Colorimetry
Counting sections of 48 Wells
Automation possible

Negative Control

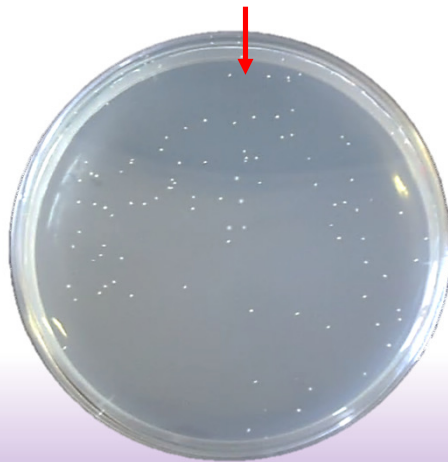


Positive Control

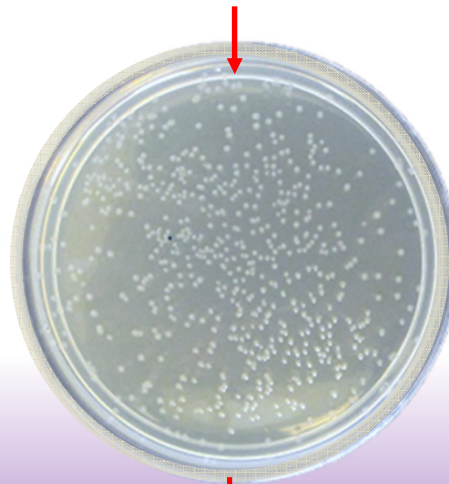

Laborious

Negative Control

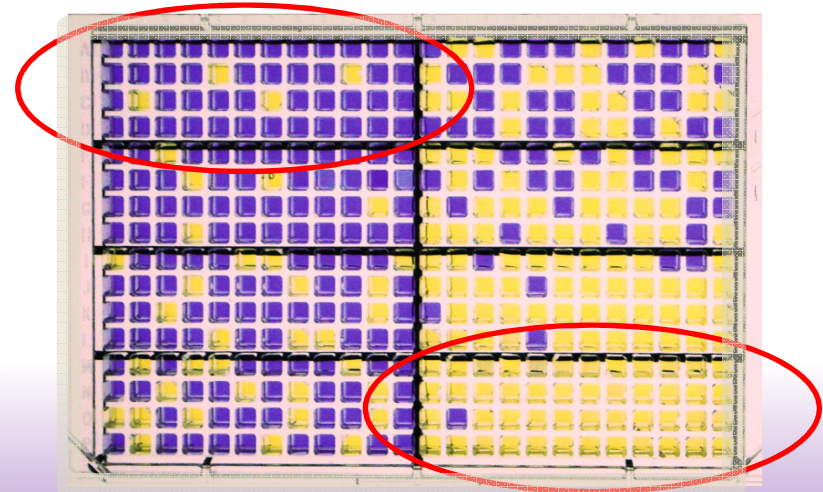

Positive Control


Easy

Throughput of compounds: Hands-on-time for 1 compound in 5 strains

1 sample, 5 concentrations, 5 strains (OECD), -/+ S9, controls, triplicates,
→ Conditions: manual handling, ready-made agar plates and top agar

	Agar Plate / 5 Conc.	MPF / 6 Conc.
Sample dilutions:	~5 min	~5 min
Top agar (preparation of tubes):	~35 min	-
Addition of sample, culture, S9:	~50 min	~25 min
Plating:	~40 min	-
Transfer to 384-well plates:	-	~40 min
Handling time:	~130 min	~70 min
Counting time:	~180 min	~20 min
Total time:	~ 5 h	~1½ h

Visualization of Plate Counting Time

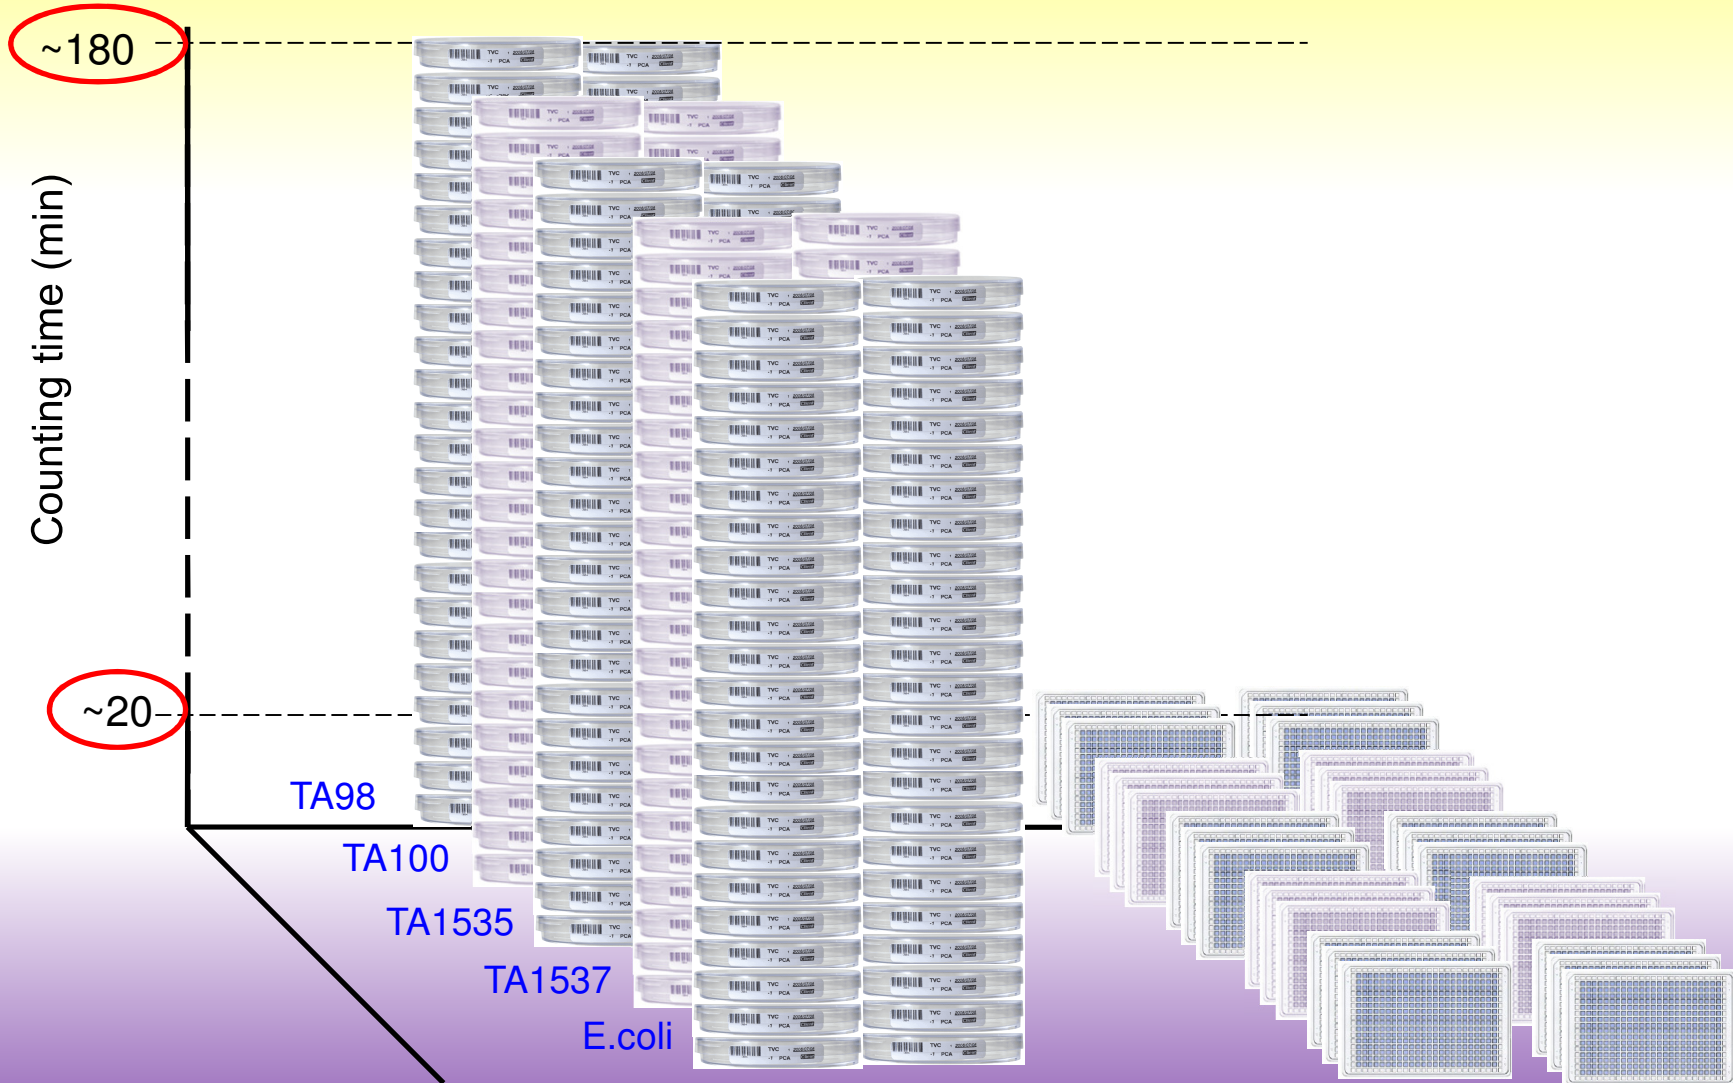

Test Sample Consumption

Minimum amount of sample needed: Agar plate test vs. Ames MPF

Setup: 5 strains (OECD 471), 1/2 log dilution steps,
triplicates, +/- S9

	<u>Ames Agar Plate:</u>	<u>Ames MPF:</u>
Top dose:	5 mg/plate	5 mg/ml
Test sample:	220 mg	55 mg

Ames MPF:

- ⇒ 4-fold less test sample
- ⇒ Very important when compound quantity is limited!
- ⇒ Genotoxic impurities

S9 Consumption

Setup: 5 strains (OECD 471), 1/2 log dilution steps, triplicates, S9

Ames Agar Plate:

S9 30%: 15.57 ml

S9 10%: **5.25 ml** - usually applied in agar plate test

Ames MPF:

1.35 ml - usually applied in Ames MPF

0.45 ml



Ames MPF:

- ⇒ **4-fold up to 11-fold less S9**
- ⇒ **Reduced number of sacrificed animals !**
- ⇒ **In line with 3Rs: Replace, Reduce, Refine !**

Critical Points of Ames MPF


- Comparability of concentrations used (mg/plate - mg/ml)?
- 48-well limit?
- Cytotoxicity?
- Colored compounds: Interference with colorimetric read-out?

Concentrations used - Comparison

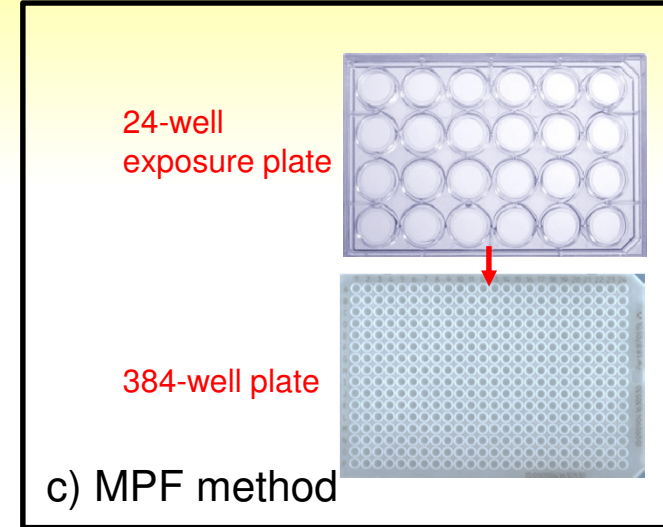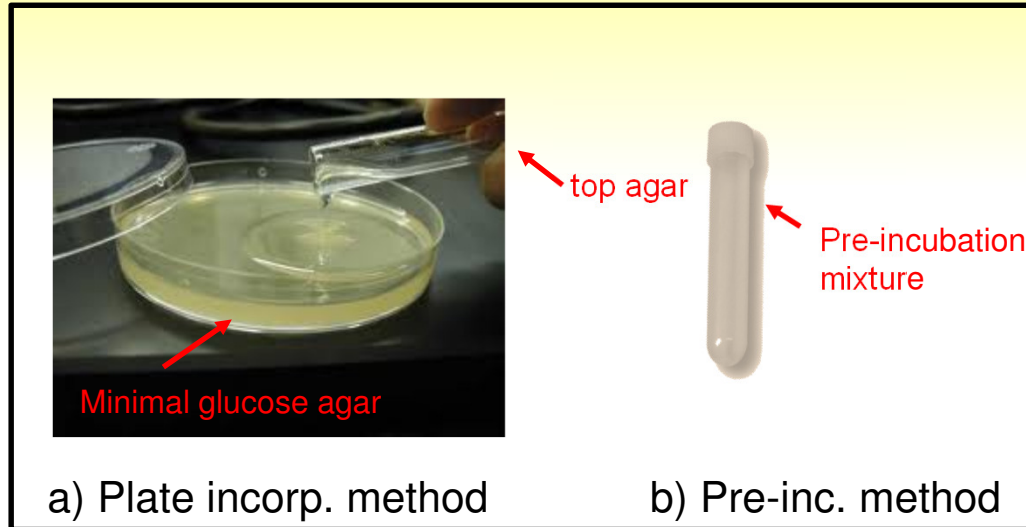

a) Plate incorporation: defined sample amount in top agar

- immediate pouring
- **possible diffusion of sample and cofactors into lower agar**
- **volume not always clearly defined during exposure**



b) Pre incubation.: defined sample amount in defined volume

- liquid pre-incubation/exposure → dilution with top agar → pouring
- **defined volume during exposure**

c) Ames MPF: defined sample amount in defined volume

- liquid exposure → dilution with indicator medium
- **defined volume during exposure**

Sample Concentration - Comparison


MPF method and Pre-incubation method: Both exposures performed in liquid media ⇒ Bacteria incubated with constant sample concentrations

Liquid exposure with 5 mg/ml (MPF) or 5 mg/plate (pre-incubation)


	Addition	Stock	Final Volume	Final concentration
MPF	10 μ l	125 mg/ml	0.25 ml	5.0 mg/ml
Pre-incubation	100 μ l	50 mg/ml	0.70 ml	7.1 mg/ml

48 Well Limit

Strong mutagens
Number of revertants




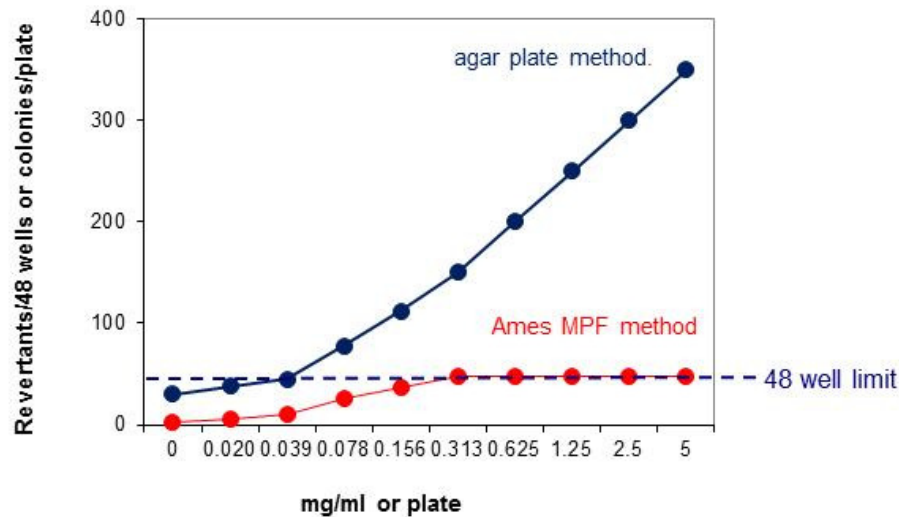


Lowest mutagenic concentration

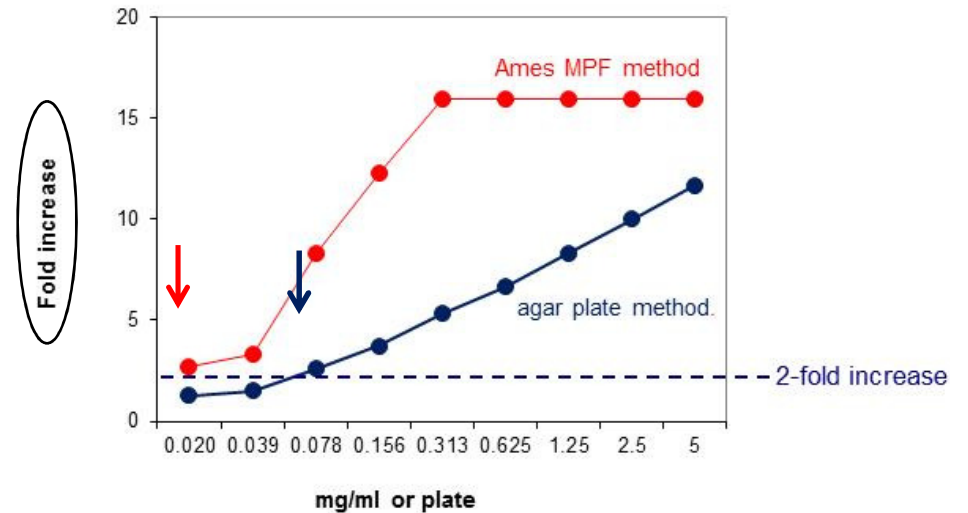

- No limits of revertants for strong mutagens in agar test, continuous increase of revertants
- Plateau of 48 wells, but: Repeated 48 revertant wells = strong mutagen in Ames MPF
- Ames MPF detects lowest mutagenic concentration at lower dose
- Low number of spontaneous revertants

Historical Solvent Control

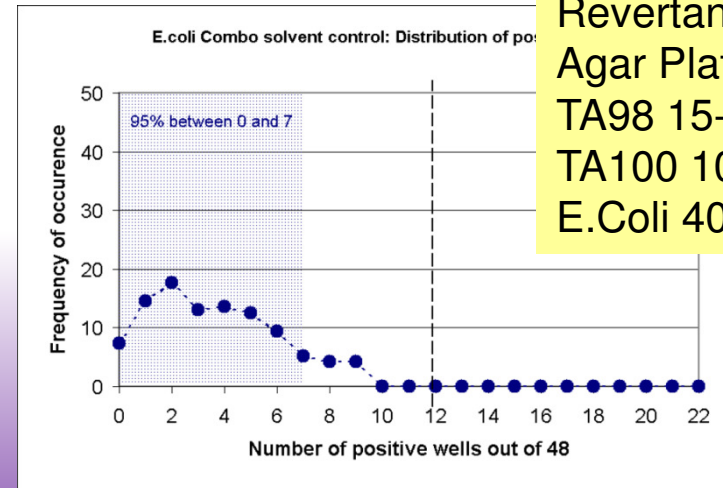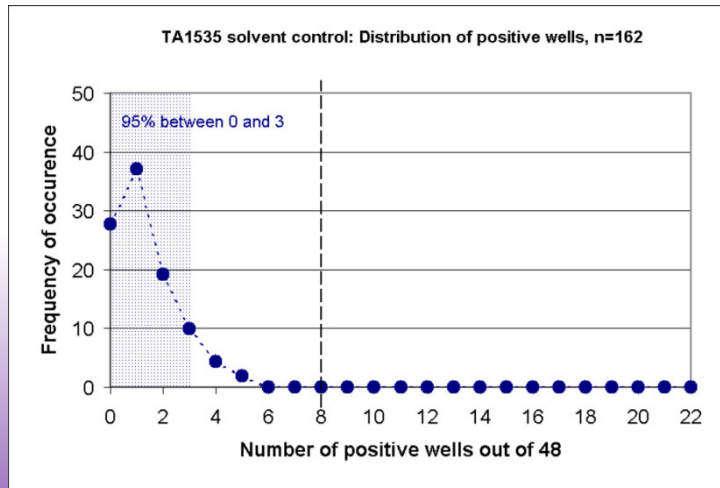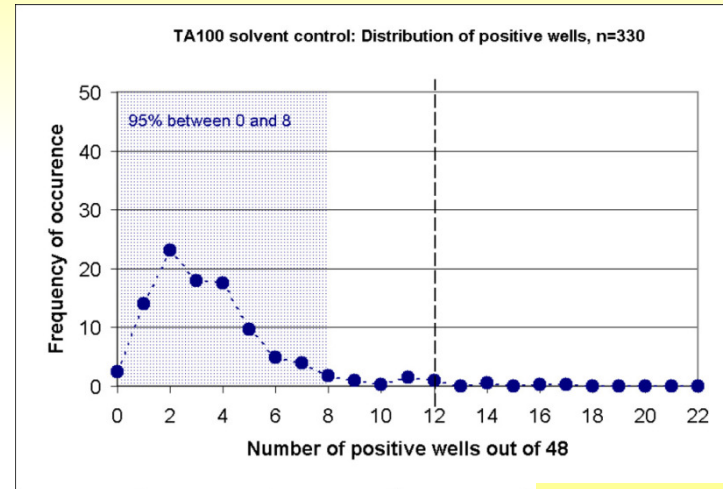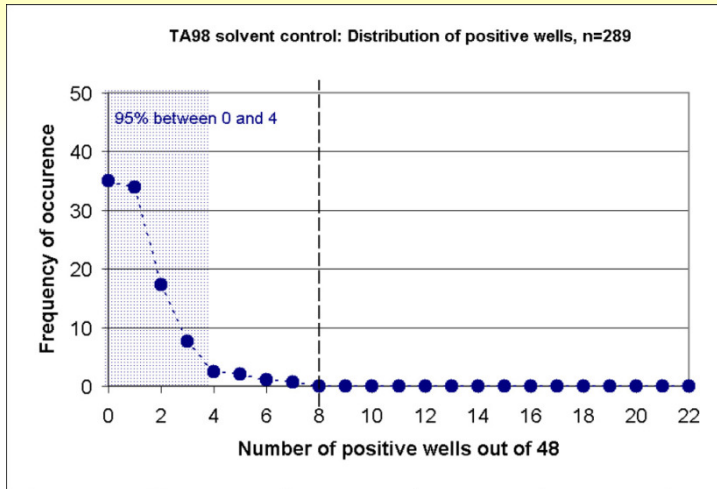


Spontaneous Revertants on Agar Plate Test
TA98 15-30
TA100 100-200
E.Coli 40-70


48 Well Limit in Ames MPF

“Low” and “High” Spontaneous Revertants

Positive Wells

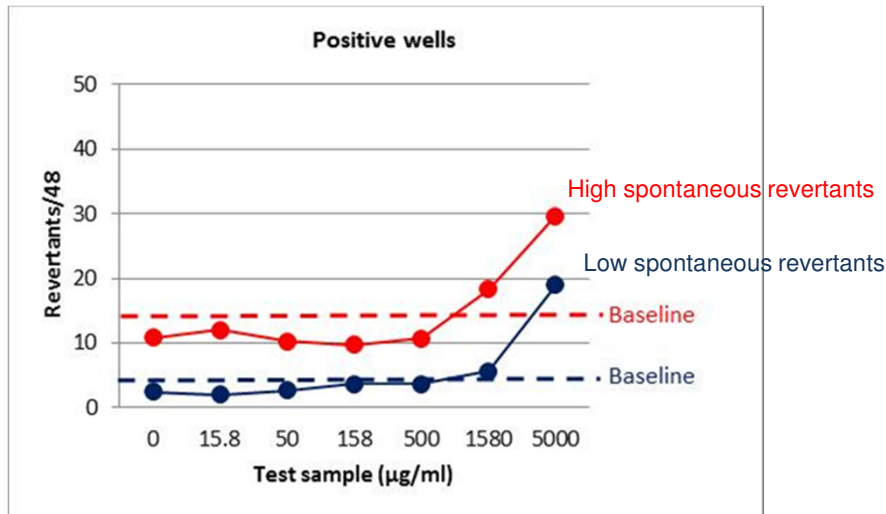

Fold Increase over Baseline

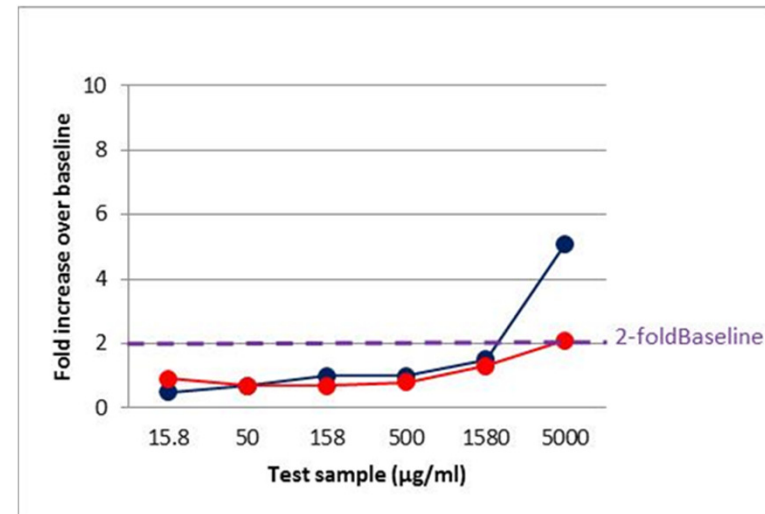

- ⇒ Pass/Fail criteria for spontaneous revertants in Ames MPF
- ⇒ Low spontaneous revertants -> larger dynamic range
- ⇒ Selection of cultures with low spontaneous revertant rate at Xenometrix, 2 quality controls after production

Cytotoxicity in Ames MPF



Cytotoxicity can be detected easily:

Reduction of revertant wells and





Increased brilliance of purple medium

Lipid droplets (bubbles) without S9

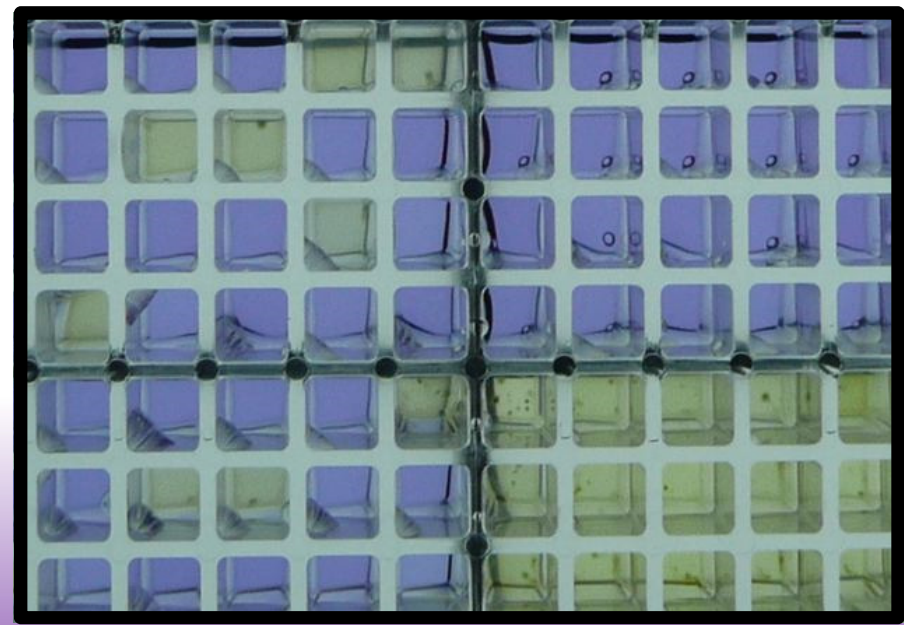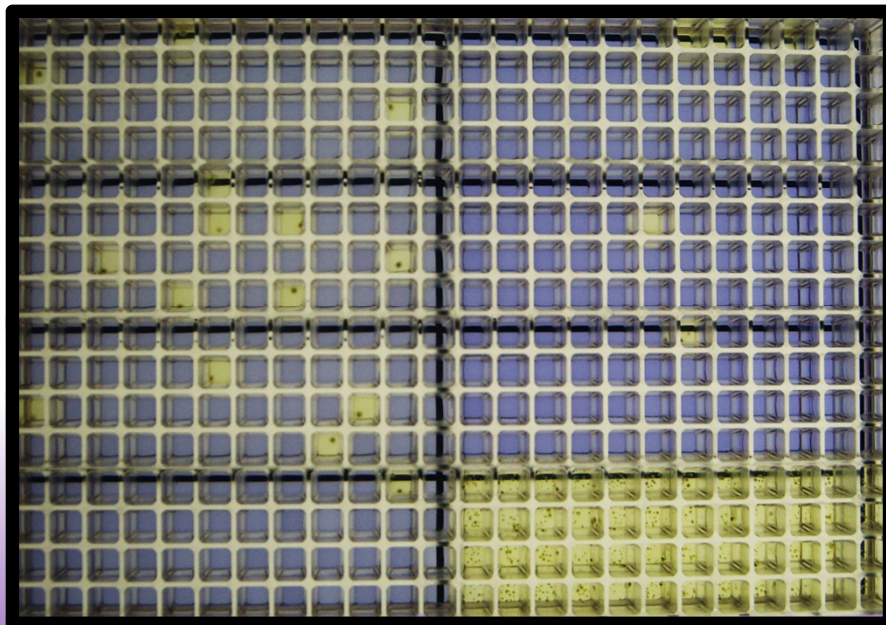

Colored compounds - colorimetric read-out

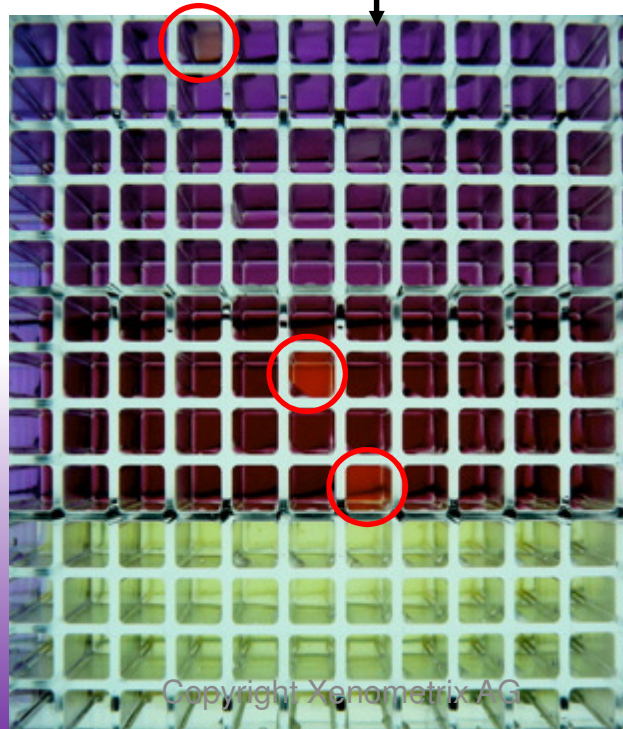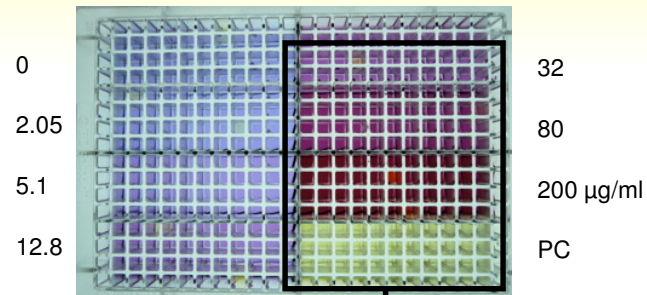

Orange instead
of yellow wells

Easily
detectable



EUROPEAN MEDICINES AGENCY
SCIENCE MEDICINES HEALTH

May 2013
EMA/CHMP/ICH/83812/2013

ICH guideline M7 on assessment and control of DNA reactive (mutagenic) impurities in pharmaceuticals to limit potential carcinogenic risk


Note 2

To assess the mutagenic potential of impurities, a single bacterial mutagenicity assay can be carried out with a fully adequate protocol according to ICH S2(R1) and OECD 471 guidelines.....**For degradants that are not feasible to isolate or synthesize or when compound quantity is limited, bacterial mutagenicity testing could be carried out using a miniaturized assay format with proven high concordance to the ICH-compliant assay** to enable testing at higher concentrations with justification.....

High concordance with agar plate test



Mutation Research 412 (1998) 115–130



Comparison of responses of base-specific Salmonella tester strains with the traditional strains for identifying mutagens: the results of a validation study

P. Gee ^{a,*}, C.H. Sommers ^a, A.S. Melick ^a, X.M. Gidrol ^a, M.D. Todd ^a,
R.B. Burris ^a, M.E. Nelson ^a, R.C. Klemm ^a, E. Zeiger ^b

TA98, TA1537, TAMix compared with all strains NTP

25 chemicals tested

Overall agreement: 88%

Abstract

The ability of a TA7000 series of Salmonella *his*⁻ mutant tester strains to detect mutagens as classified by the traditional

High concordance with agar plate test



Available online at www.sciencedirect.com

SCIENCE @ DIRECT®

Mutation Research 558 (2004) 181–197

MR

Genetic Toxicology and
Environmental Mutagenesis

www.elsevier.com/locate/genotox

Community address: www.elsevier.com/locate/mutres

Assessment of the performance of the Ames II™ assay: a collaborative study with 19 coded compounds

S. Flückiger-Isler^{a,*}, M. Baumeister^b, K. Braun^c, V. Gervais^d, N. Hasler-Nguyen^e,
R. Reimann^f, J. Van Gompel^g, H.-G. Wunderlich^h, G. Engelhardtⁱ

^a *Xenometrix by Endotell GmbH, CH-4125 Aalschwil, Switzerland*

^b *Boehringer Ingelheim, Department of Non-Clinical Drug Safety, Boehringer Ingelheim Pharma KG & Co. KG,
D-88397 Biberach, Germany*

^c *Aventis Pharma Deutschland GmbH, Drug Innovation & Approval, Lead Optimization, Drug Safety Evaluation,
D-65795 Hattersheim, Germany*

^d *Servier Group, Drug Safety Assessment, F-45403 Orléans-Gidy, France*

^e *Novartis Consumer Health, Toxicology, CH-1260 Nyon, Switzerland*

^f *Schering AG, Experimental Toxicology, D-13342 Berlin, Germany*

^g *Johnson&Johnson Pharmaceutical Research & Development, Department of ADME/Tox, B-2340 Beerse, Belgium*

^h *Federal Environmental Agency, Department for Hygiene of Drinking and Swimming Pool Water, D-08645 Bad Elster, Germany*

Overall agreement standard Ames (all strains) - Ames II (TA98, TAMix):
84.2% (16/19)

Inter-laboratory consistency of 89.5% (17/19).

High concordance with agar plate test

ASSESSMENT OF A SCREENING EXPERIENCE WITH THE AMES II™ TEST AND FUTURE PROSPECTS

V. GERVAIS¹, D. BIJOT¹ and N. CLAUDE²

¹ Drug Safety Assessment, Sanvier, Orléans-Gdy, France, ² IRIS, Sanvier, Coubarcia, France

quid fluctuation version of the *Salmonella* mutagenicity assay, provided by Xenometrix GmbH, was used for an early compound selection in the discovery process. The aim was to compare the Ames II to the standard Ames test and to explore a way to reduce the required compound quantity without lowering the predictability of the test.

METHODS

A mixture of 6 *Salmonella* strains (TA7001, TA7002, TA7003, TA7004, TA7005, TA7006), which revert to a specific base substitution (G to A), is used as a reference strain. This "mix" is used as a reference strain. The frameshift tester strain mix and TA98 strains are used for growth overnight at 37°C, performed in 24-wells plates. The Ames II test was performed with partial automation and about 60-fold less compound than the standard Ames. After a 90 min incubation with or without Aroclor-induced solvent and positive medium lacking histidine is then aliquoted into 24-wells plates.

Tab.1: Results of a collaborative study by Xenometrix GmbH (March 2003)

Company	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20
G1	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P
G1 (Revised)	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P
U1	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U2	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U3	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U4	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U5	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U6	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U7	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U8	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U9	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U10	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U11	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U12	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U13	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U14	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U15	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U16	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U17	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U18	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U19	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
U20	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N	N
Ames II	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P
Ames I	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P	P

Sensitivity : 83%
Specificity : 100%
Concordance : 88%

RESULTS

350 compounds were tested, including molecules from our own research, known non- or genotoxins producing equivocal results. The concordance between the results achieved with the Ames II™ test and those reported in the literature for the standard Ames test ranged from 79% (Ref. 1) to 89% (Tab.2). The concordance reached 88% in this collaborative study (Tab.1). No false positives were obtained with known non-mutagenic compounds. False negative results may arise when chemically active compounds like TA1535 or *E. coli* (pKM101) which meet no equivalent in the Ames II™ test. The positive responses were randomly distributed among the strains or the concentration range tested. In contrast, only 11% of positive results were specifically in the absence of S9 (Fig.4), which is not the case for the Ames II™ test.

83% Concordance Ames II vs. traditional Ames using 42 company-owned chemicals (disagreement mainly with compounds that specifically revert *E. coli*, TA1535)

No false positive results

High concordance with agar plate test

Mutagenesis vol. 24 no. 4 pp. 359–366, 2009
Advance Access Publication 15 May 2009

doi:10.1093/mutage/geb017

Comparison of the Ames II and traditional Ames test responses with respect to mutagenicity, strain specificities, need for metabolism and correlation with rodent carcinogenicity

Markus Kamber*, Sini Flückiger-Isler,
Günter Engelhardt¹, Rudolf Jaeckh² and Errol Zeiger³

Xenometrix AG, Gewerbestrasse 25, CH-4123 Allschwil, Switzerland,
¹Experimental Toxicology and Ecology, BASF SE Product Safety,
²Regulations, Toxicology and Ecology, BASF SE Product Safety, 67056
Ludwigshafen am Rhein, Germany and ³Errol Zeiger Consulting, Chapel Hill,
NC 27514, USA


The Ames II *Salmonella* mutagenicity assay procedure was used to test 71 chemicals, and the results were compared with those from the traditional Ames *Salmonella* test using the NT format.

84% agreement between the two procedures in identifying mutagens and non-mutagens
Discordant results included chemicals requiring reductive metabolism using FMN, hamster liver S9

a different test method, including a simple, overall agreement or disagreement; agreement or disagreement with regard to the genetic endpoint, and whether metabolic activation is required for activity; comparisons of the active test chemical concentration ranges and with respect to the effect the test is designed to predict, i.e. cancer. Two previous studies (3,4) have compared the performance of the Ames II assay to that of the traditional Ames test procedure [i.e. the procedure with the traditional strains, as described in (5) and (6)] to validate its use as an alternative to the traditional Ames test procedure.

High concordance with agar plate test

Xenometrix Posters: Comparison with Correspondent Traditional Strains

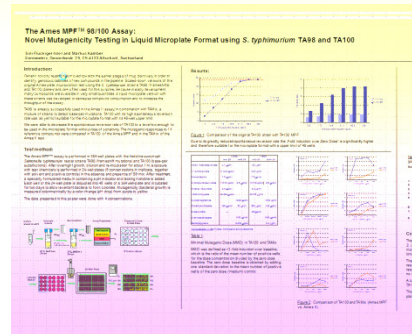

- TAMix vs. TA100 MPF and TA100 published traditional Ames
- TA98, TA100, TA1535, TA1537 MPF vs. TA98, TA100, TA1535, TA1537 published traditional Ames
- Ames MPF PENTA I (strains as above plus EC Combo) vs. published traditional Ames

⇒ Overall agreement: 89 - 100%

High concordance with agar plate test

Direct Comparison Ames MPF - Ames Pre-incubation

Mutation Research 747 (2012) 36–45



Contents lists available at SciVerse ScienceDirect
**Mutation Research/Genetic Toxicology and
Environmental Mutagenesis**

journal homepage: www.elsevier.com/locate/gentox
Community address: www.elsevier.com/locate/mutres



Direct comparison of the Ames microplate format (MPF) test in liquid medium with the standard Ames pre-incubation assay on agar plates by use of equivocal to weakly positive test compounds







Sini Flückiger-Isler*, Markus Kamber

Xenometrix AG, Allschwil, CH-4123 Allschwil, Switzerland

- 15 equivocal to weakly positive chemicals
- Same overnight cultures, chemicals and S9 to exclude external variations, i.e. culture growth, chemical purity, weighing errors, S9 activity
- Parallel tests with most responsive strains of the NTP database (mg/plate vs. mg/ml)
- Each test was repeated at least once
- 87% concordance (13/15)
- Excellent concordance for equivocal to weak positive chemicals
- Confirms the high concordance with the ICH-compliant assay

Direct Comparison Ames MPF and Pre-incubation Method (see publication before)

$\mu\text{g/ml}$ vs. $\mu\text{g/plate}$

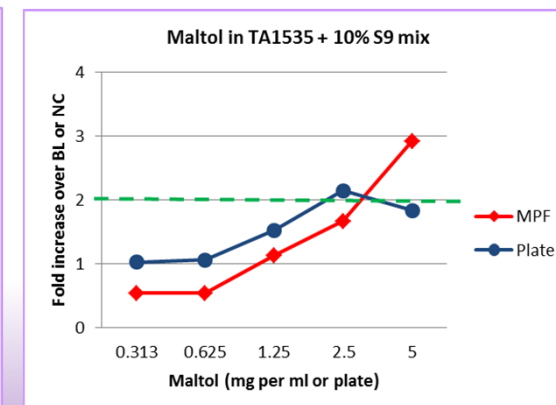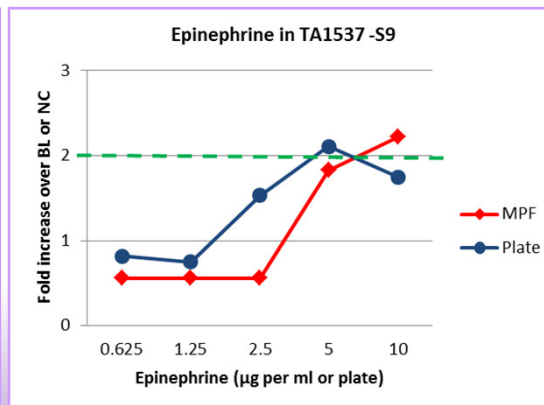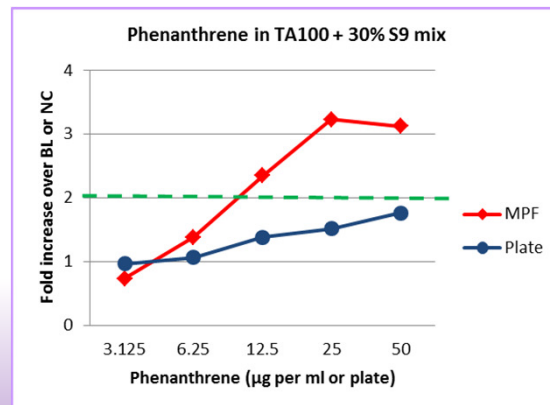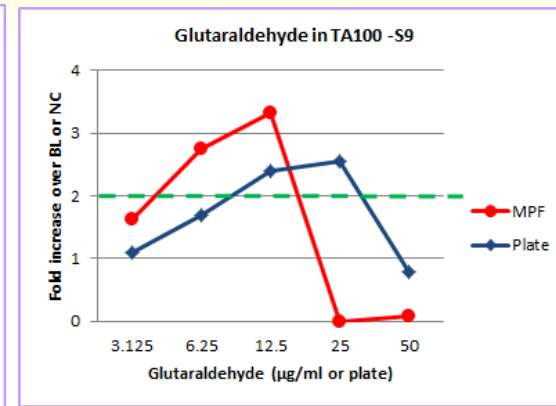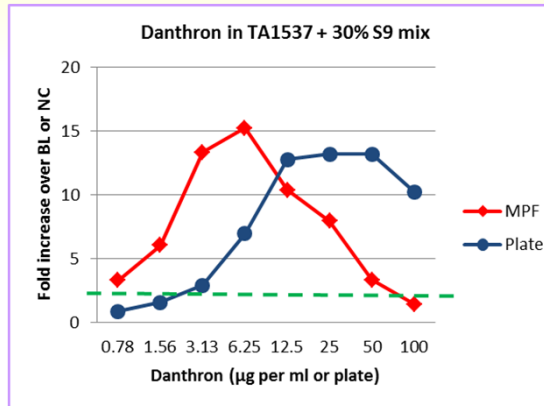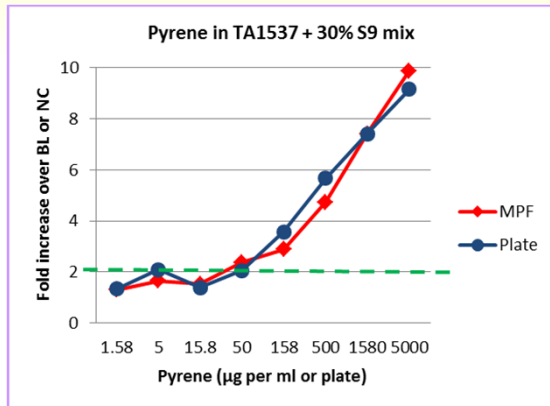

Higher sensitivity of Ames MPF with several compounds, such as Danthron, Glutaraldehyde, Phenanthrene





At first glance higher sensitivity of Pre Incubation Assay with Maltol and Epinephrine, but....

Direct Comparison Ames MPF and Pre-incubation Method – Epinephrine, Maltol

Correction for concentration in preincubation assay (5.0 mg vs 7.1 mg)


µg/ml vs. µg/plate

µg/ml vs. µg/ml (pre-incubation volume 0.7 ml)

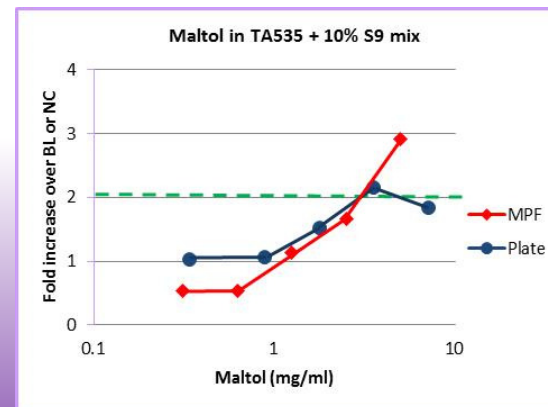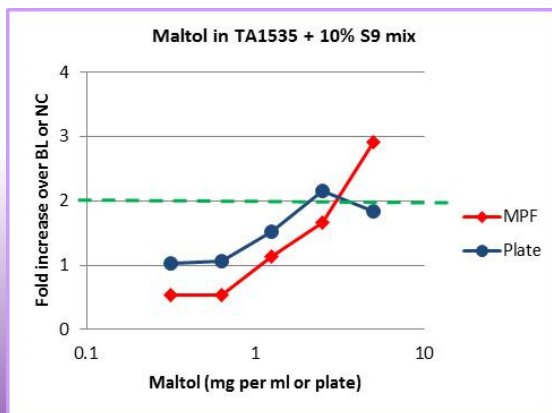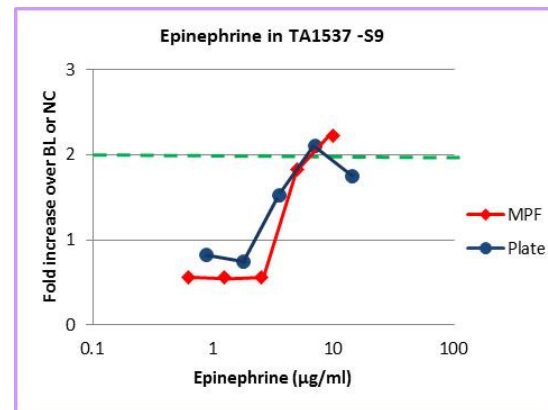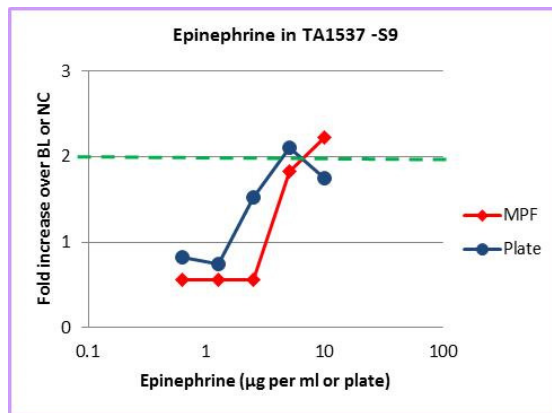

Congruent curves

Ames MPF is a very sensitive assay

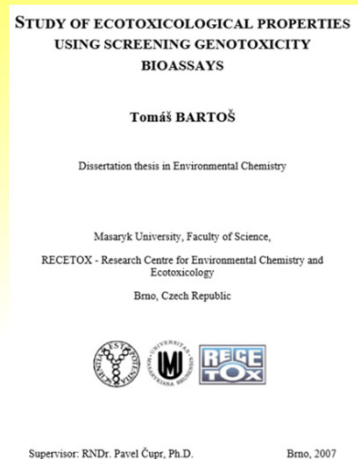

Chapter 5

Perspectives in genotoxicity screening

“Ames II (Xenometrix, Switzerland) is a microplate-based fluctuation test version of the Ames test and probably the best Ames predictor.”




Chapter 9: Mutation Research




New Paradigms for the Environmental Assessment, p. 26

“Thus, the all-liquid format of the Ames II/MPF assay, which requires less test compound and allows for the use of multichannel pipettes, thus automating the pipetting steps, makes this procedure an attractive method to evaluate mutagenicity of a large number of samples at the same time - a common situation in environmental monitoring”.

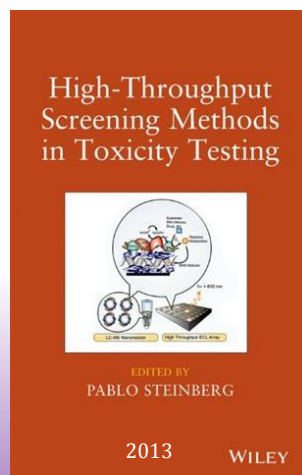

Chapter 10: Ames II and Ames Liquid Format Mutagenicity Screening Assays

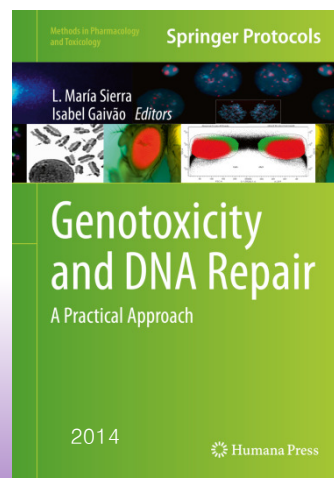

Chapter 2: The Ames II and Ames MPF Penta I Assay: A Liquid Microplate Format Modification of the Classic Ames Test



..it has been proposed by the European Union-funded REBECA project as a screening tool to determine whether fungal biological control agents produce genotoxic/mutagenic metabolites which require further attention in the regulatory risk assessment.

Conclusion I - Test Performance

- Ames MPF – Ames agar test: same principle, same tester strains
- Comparative studies: mean concordance of ~87%
- Comparable to the intra- and inter-laboratory reproducibility of the agar plate Ames test procedure

Conclusion II

Advantages

- 4 x less test sample necessary
- Liquid microplate format allows for less hands-on-time, simultaneous processing of several replicates
- Higher throughput, partly automatable
- 12 fold less consumption of S9 – following 3Rs
- Quick, easy colorimetric read-out, less error prone
- Less plastic ware, reduced contaminated waste in environment
- Listed explicitly in ICH M7 Guideline
- **Higher Sensitivity – depending on compound**



Disadvantages

- Not same large database as agar plate method
- Not listed explicitly in OECD 471



Conclusion III - ICH Guideline M7

- The Ames MPF features a miniaturized assay format with proven high concordance with the ICH-compliant assay.
- It is highly sensitive and allows testing compounds present in limited quantity.

⇒ Ames MPF = Excellent tool for assessing mutagenic impurities

ASSESSMENT AND CONTROL OF DNA REACTIVE (MUTAGENIC)
IMPURITIES IN PHARMACEUTICALS TO LIMIT POTENTIAL
CARCINOGENIC RISK

M7

“For degradants that are not feasible to isolate or synthesize or when compound quantity is limited, it may not be possible to achieve the highest test concentrations recommended for an ICH compliant bacterial mutagenicity assay according to the current testing guidelines. In this case, bacterial mutagenicity testing could be carried out using a miniaturized assay format with proven high concordance to the ICH compliant assay to enable testing at higher concentrations with justification.....”